



ZYMO RESEARCH

DNA  
Purification  
*MAKING DNA*  
Made Simple™

## Select-a-Size DNA Clean & Concentrator™ MagBead Kit

Purify desired range of DNA fragment sizes from library preps, PCR, endonuclease digestions, ligations, etc.

### Highlights

- **Tunable:** High quality tunable DNA fragment size selection 150–800 bps
- **Consistent Performance:** Rapid purification with high reproducibility
- **Automation Ready:** Automation friendly and scalable protocol

Catalog Numbers:  
D4084, D4085



Scan with your smart-phone camera to  
view the online protocol/video.



[tech@zymoresearch.com](mailto:tech@zymoresearch.com)



[www.zymoresearch.com](http://www.zymoresearch.com)



Toll Free: (888) 882-9682

# **Table of Contents**

---

<b>Product Contents</b> .....	<b>01</b>
<b>Specifications</b> .....	<b>02</b>
<b>Product Description</b> .....	<b>04</b>
<b>Protocol</b> .....	<b>05</b>
Buffer Preparation.....	<b>05</b>
Clean-up and Left-Sided Size Selection....	<b>05</b>
Right-Sided Size Selection .....	<b>07</b>
Double-Sided Size Selection.....	<b>09</b>
<b>Troubleshooting</b> .....	<b>10</b>
<b>Appendix</b> .....	<b>13</b>
<b>Ordering Information</b> .....	<b>14</b>
<b>Guarantee</b> .....	<b>15</b>

# Product Contents

Select-a-Size DNA Clean & Concentrator™ MagBead Kit	D4084 (10 ml)	D4085 (50 ml)	Storage Temperature
Select-a-Size MagBeads	10 ml	50 ml	4–8 °C
DNA Wash Buffer <sup>1</sup>	24 ml	3 x 24 ml	Room Temp.
DNA Elution Buffer	16 ml	50 ml	Room Temp.
Instruction Manual	1	1	-


**Note:** Plates and consumables, sold separately. See page 14.

---

<sup>1</sup> Ethanol must be added prior to use as indicated on **DNA Wash Buffer** label.

# Specifications

- **DNA Purity** – Eluted DNA is of high quality and is well suited for ligations, restriction digestions, library preparation cleanup, and next generation sequencing applications.
- **Recovery Volume** –  $\geq 25 \mu\text{l}$  of **DNA Elution Buffer** for 96 well plates.  $\geq 10 \mu\text{l}$  of **DNA Elution Buffer** for manual preps performed using microcentrifuge tubes.
- **Required Equipment** – Magnetic Separator
- **Processing Time** –  $\geq 10$  mins
- **Principle of Technology** – The **Select-a-Size DNA Clean & Concentrator™ MagBead Kit** works on the principle of selective binding, wherein the size of the nucleic acid and the ratio of the magnetic beads controls what is retained on the beads and what remains in the supernatant. Either fraction (beads or supernatant) can be further purified which is an enabling and flexible feature of this technology. As the ratio of MagBeads to sample increases, proportionally lower molecular weight DNA (smaller fragments) are retained. Therefore, the size selection is controlled by increasing or decreasing quantities of MagBeads. Samples can be size selected to remove smaller fragments with Left-Sided Size Selection, larger fragments with Right-Sided Size Selection (**Figure 1**), or both large and small fragments in Double-Sided Size Selection. Listed within this protocol are the most common cutoffs and starting sample volumes. Cutoffs not included within this protocol can be determined by titrating between points.

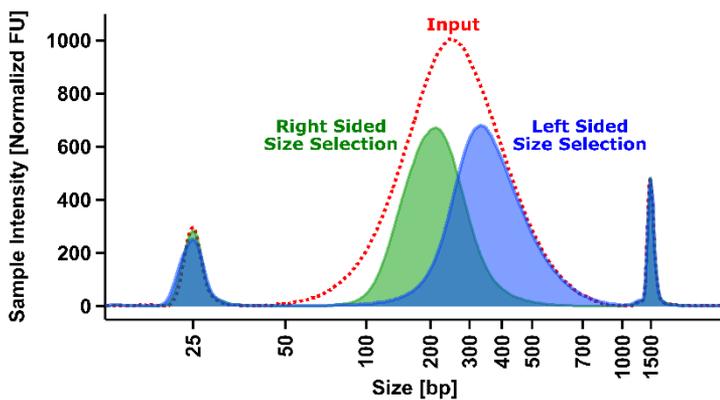


**Figure 1.** Right sided (green) and left sided (blue) selection on sonicated salmon sperm DNA (red) DNA size was selected according to the Select-a-Size DNA Clean & Concentrator™ MagBeads protocol and the results were analyzed by Agilent 4150 TapeStation. 50  $\mu$ l of sonicated salmon sperm DNA at a concentration of 8.0 ng /  $\mu$ l in water was used as a standard input to evaluate size selection efficiency and cutoff.

# Product Description

The **Select-a-Size DNA Clean & Concentrator™ MagBead Kit** provides the fastest and easiest method to purify specific ranges of DNA fragments from PCR, endonuclease digestions, ligations, library preparations, adapter removal, etc. This simple workflow allows for specific cutoffs that can be modified to suit reaction clean-up, left-sided, right-sided or even double-sided size selection. The **Select-a-Size MagBeads** selectively binds fragments based on the volume added relative to the sample. Simply choose a desired cutoff to bind the target of interest onto the beads and remove species outside of this range. (**Figure 2**) The desired DNA is easily eluted from the beads following a rapid wash regimen.

Choose from one of the pre-determined cutoffs or fine-tune the protocol for even more specific selections between these points. Size selections can be performed in as little as 10 minutes to yield high-quality DNA which is suitable for highly sensitive applications including Next Generation Sequencing, and any other sensitive downstream applications. The protocol can be performed manually or using an automated platform for high throughput processing.

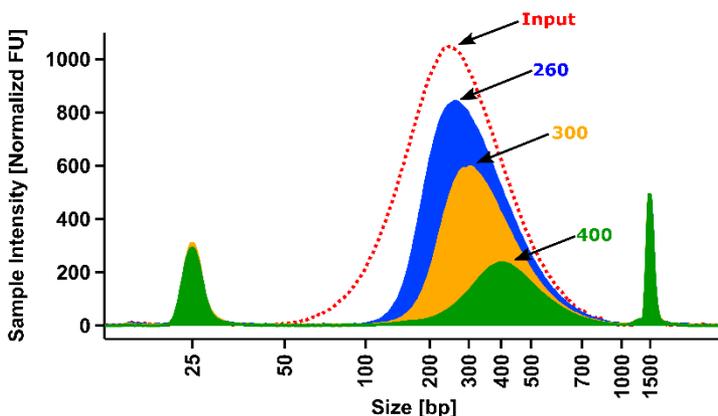

**Figure 2.** Select-a-Size DNA Clean & Concentrator™ MagBead Kit demonstrating left-sided size selection at 260 bp (blue trace), 300 bp (yellow trace), 400 bp (green trace). DNA size was selected according to the Select-a-Size DNA Clean & Concentrator™ MagBead kit protocol and the results were analyzed by Agilent 4150 TapeStation. 50  $\mu$ l of sonicated salmon sperm DNA at a concentration of 9.0 ng /  $\mu$ l in water was used as a standard input to evaluate size selection efficiency and cutoff.

# Protocol

## Buffer Preparation

*Before starting:* Add 96 ml of 100% ethanol (104 ml 95% ethanol) to the 24 ml **DNA Wash Buffer** concentrate.

## Clean-up and Left-Sided Size Selection (Depletion of Small Fragments):

*The following procedure should be performed at room temperature (20–30°C).*

1. Resuspend the magnetic particles by vigorously shaking the **Select-a-Size MagBeads** until homogenous.<sup>1</sup>
2. Choose the desired peak from the **Table 1** below.<sup>2</sup> For a sample volume of 50 µL, determine the amount of **Select-a-Size MagBeads** required.

Note: (Sample Volume) x (Ratio) = Volume of Select-a-Size MagBeads

**Table 1.** This table shows the recommended titration volumes for a 50 µL sample to retain the peak DNA fragments listed.

Peak DNA Fragments Retained	Ratio of Select-a-Size MagBeads	Volume of MagBeads for 50 µl starting sample
260	1.24	62
300	0.98	49
400	0.76	38

3. Add the necessary volume of **Select-a-Size MagBeads** to the sample. Mix thoroughly by pipetting or vortexing until homogenous. Incubate for 5 minutes at up to 30 °C.<sup>3</sup>
4. Place the sample on a magnetic rack or plate and incubate for 5 minutes, or until the magnetic beads have fully separated from solution.
5. Once the beads have been cleared from solution, remove and discard the supernatant.<sup>4</sup>

<sup>1</sup> For complete resuspension, allow **Select-a-Size MagBeads** to equilibrate to room temperature (20-30°C).

<sup>2</sup> For complete adapter/dimer removal, select a cutoff that is at least 50 bp above the undesired fragment size.

<sup>3</sup> For maximum recovery and consistent yields, incubation at 30 °C is recommended but not required at any step.

<sup>4</sup> Avoid aspirating any beads when removing the supernatant. To best prevent this, leave 2-5 µl of liquid in the sample container.

6. While the beads are still on the magnetic rack, add 200  $\mu\text{l}$  of **DNA Wash Buffer**. Remove and discard the supernatant. Repeat this step.
7. While the beads are still on the magnetic rack, aspirate any residual **DNA Wash Buffer**. Remove samples from the magnetic rack.<sup>5</sup>
8. Add  $\geq 25 \mu\text{l}$  **DNA Elution Buffer** to the beads<sup>6,7</sup> and mix thoroughly by pipetting up and down or vortexing until homogenous. Incubate at up to 30 °C for 2 minutes.
9. Place the sample on a magnetic rack for 1–2 minutes to separate the magnetic beads from eluate.
10. Transfer supernatant to a clean microcentrifuge tube or 96-well plate. The ultrapure DNA is now ready for use.

---

<sup>5</sup> An optional drying incubation of 3 minutes at room temperature can be performed to ensure all traces of ethanol are removed.

<sup>6</sup> For plates, an elution volume greater than 25  $\mu\text{l}$  may be required to guarantee full contact with the magnetic beads.

<sup>7</sup> For microcentrifuge tubes, an elution volume as low as 10  $\mu\text{l}$  can be used to resuspend the beads and obtain a highly concentrated eluate.

## **Right-Sided Size Selection (Depletion of Large Fragments):**

**Important!** See **Buffer Preparation** on page 5 before starting.

The following procedure should be performed at room temperature (20–30 °C).

1. Resuspend the magnetic particles by vigorously shaking the **Select-a-Size MagBeads** until homogenous.<sup>1</sup>
2. Bring the DNA sample volume up to 50 µl with **DNA Elution Buffer**.
3. Choose the desired cutoff from **Table 2** below. Add the necessary volume of **Select-a-Size MagBeads** to the sample based on the desired ratio. Mix thoroughly by pipetting or vortexing until homogenous. Incubate this mixture for 5 minutes at up to 30 °C.<sup>2</sup>

Note: (Sample Volume) x (Ratio) = Volume of Select-a-Size MagBeads

**Table 2.** This table shows the recommended titration volumes for a 50 µL sample to deplete DNA fragments above the size listed.

DNA Fragments depleted	First Ratio of Select-a-Size MagBeads	First Volume of MagBeads
>200	0.96	48
>300	0.80	40
>400	0.72	36
>600	0.60	30
>700	0.56	28

4. Place the sample on a magnetic rack or plate and incubate for 5 minutes, or until the magnetic beads have fully separated from solution.
5. Once the beads have been cleared from solution, **transfer the supernatant into a new tube**.<sup>3</sup> Discard the beads.
6. Refer to **Table 3** and add the necessary volume of **Select-a-Size MagBeads** to the supernatant from step 5 based on the cutoff chosen in step 3. Mix thoroughly by pipetting or vortexing until homogenous. Incubate this mixture for 2 minutes at up to 30 °C.

Example: To retain fragments smaller than 300 bp with a 50 µl starting sample, add 50.0 µl to the supernatant from step 5.

<sup>1</sup> For complete resuspension, allow **Select-a-Size MagBeads** to equilibrate to room temperature (20-30°C).

<sup>2</sup> For maximum recovery, mix samples well and incubate samples for 5 minutes.

<sup>3</sup> Avoid aspirating any beads when removing the supernatant. To best prevent this, leave 2-5 µl of liquid behind.

**Table 3.** This table shows the recommended titration volumes to recover the desired fragments retained in the supernatant from the previous step.

DNA Fragments depleted	Second Ratio of Select-a-Size MagBeads	Second Volume of MagBeads
>200	0.47	42
>300	1.00	50
>400	1.08	54
>600	1.20	60
>700	1.24	62

7. Place the sample on a magnetic rack or plate and incubate for 5 minutes, or until the magnetic beads have separated from solution.
8. Once the beads have cleared from solution, discard the supernatant.<sup>4</sup>
9. While the beads are still on the magnetic rack, add 200  $\mu$ l of **DNA Wash Buffer**. Remove and discard the supernatant. Repeat this step.
10. While the beads are still on the magnetic rack, aspirate any residual **DNA Wash Buffer**. Remove samples from the magnetic rack.<sup>5</sup>
11. Add  $\geq$  25  $\mu$ l **DNA Elution Buffer** to the beads<sup>6, 7</sup> and mix thoroughly by pipetting up and down or vortexing until homogenous. Incubate at up to 30 °C for 2 minutes.
12. Place the sample on a magnetic rack and incubate for 2 minutes, or until the magnetic beads have separated from solution.
13. Transfer supernatant to the final tube or plate. The ultra-pure DNA is now ready for use.

<sup>4</sup> Avoid aspirating any beads when removing the supernatant. To best prevent this, leave 2-5  $\mu$ l of liquid behind.

<sup>5</sup> An optional drying incubation of 3 minutes at room temperature can be performed to ensure all trace of ethanol is removed.

<sup>6</sup> For plates, an elution volume greater than 25  $\mu$ l may be required to guarantee full contact with the magnetic beads.

<sup>7</sup> For microcentrifuge tubes, an elution volume as low as 10  $\mu$ l can be used to resuspend the beads and obtain a highly concentrated eluate.

## **Double-Sided Size Selection:**

**Important!** See **Buffer Preparation** on page 5 before starting.

*The following procedure should be performed at room temperature (20–30°C).*

1. To perform a double-sided selection, choose the left-sided selection ratio and the right-sided selection ratio from the **Tables 1–3** above or as determined by titration.
2. Perform the right-sided selection according to the steps on page 7–8; elute from the bead at a 50  $\mu\text{L}$  volume with **DNA Elution buffer** for the right sided selection.
3. Perform a left-sided selection on the sample retained from the right sided selection according to the steps on page 5–6. Elute with **DNA Elution buffer** to the final desired volume.
4. Transfer supernatant to the final tube or plate. The ultra-pure DNA is now ready for use.

# Troubleshooting

Problem	Possible Causes and Suggested Solutions
<b>Choosing Your Cutoff</b>	
<i>Titrating New Peaks or Cutoffs</i>	<ul style="list-style-type: none"><li>• Alternative cutoffs can be identified by fine adjustments of the volume of <b>Select-a-Size MagBeads</b> added to the sample. The peaks and cutoffs provided within the protocol can be used as a guideline to pinpoint more specific cutoffs. In general, as the ratio of <b>Select-a-Size MagBeads</b> to sample increases, the peak or cutoff shifts to the left.</li></ul>
<b>Inaccurate Size Selection</b>	
<i>Inconsistent Size Selection</i>	<ul style="list-style-type: none"><li>• <b>Select-a-Size MagBeads not mixed thoroughly with sample.</b> Be sure to mix the MagBeads with the sample very well by pipetting or vortexing until homogenous.</li><li>• <b>Stray Droplets.</b> Cutoffs can be very sensitive to slight changes in the ratio of <b>Select-a-Size MagBeads</b> to sample for cutoffs at higher molecular weights. Be vigilant of stray droplets being carried over into the sample.</li><li>• <b>Volume of sample.</b> The sample volume should be at least 50 <math>\mu\text{l}</math> before adding <b>Select-a-Size MagBeads</b>. A lower volume is more prone to effects from pipetting inaccuracy which shifts the size selection.</li></ul>
<i>Tailing of large size range in Right/Double-Sided Size Selection</i>	<ul style="list-style-type: none"><li>• <b>Incomplete Separation.</b> Allow magnetic beads to completely separate from solution before aspirating out any liquid. The solution should be completely clear with a pellet of beads on the side of the <b>tube</b>. Take care not to aspirate out any beads in the first supernatant removal. At this step, the larger fragments are bound onto the beads. To avoid removing these beads, leave 2-5 <math>\mu\text{l}</math> of buffer behind during the first supernatant removal.</li></ul>
<i>Inefficient removal of undesired smaller fragments</i>	<ul style="list-style-type: none"><li>• <b>Incomplete Washing.</b> The undesired small fragments may be present within the wells of the <b>tube/well</b>. To remove these fragments, be sure to perform both wash steps with DNA Wash Buffer thoroughly.</li><li>• <b>Pipette Calibration.</b> Higher cutoffs can be highly sensitive to minor errors in pipetting. Ensure that pipettes are properly calibrated before performing protocol.</li></ul>

---

**Low DNA Recovery**

---

*DNA Wash Buffer*

- Ethanol was not added to the **DNA Wash Buffer**.
- **Ensure that the bottle cap is screwed on tightly** after each use to prevent evaporation of the ethanol over time.

---

*Magnetic Separation*

- **Incomplete Separation.** Allow magnetic beads to completely separate from solution before aspirating out any liquid. The solution should be completely clear with a pellet of beads on the side of the **tube**. Take care not to aspirate out any beads as the fragments of interest are bound on the beads.

---

*Inefficient Elution*

- **Elution volume does not cover the beads.** The minimum elution volume for plates will vary based on the magnetic rack used. The level of the eluate should completely cover the magnetic beads for complete elution.
- **Elution volume not large enough.** Decreasing the elution volume can lead to a decrease in the recovery. The smaller the elution volume, the more difficult it will be to aspirate the eluate without carrying beads.
- **Beads not resuspended.** When performing the elution with small volumes, it is critical to locate the pellet and resuspend the magnetic beads.

---

*Drying Time*

- **Do not over dry the MagBeads.** For complete removal of ethanol, resuspend samples with **DNA Elution Buffer** within three minutes of drying. Extended drying times reduce the elution efficiency of the beads.

---

*Inefficient Binding*

- **Mix sample with MagBeads well and incubate for at least 2–5 minutes.** To maximize the recovery of DNA, samples should be mixed thoroughly and can be incubated at 30 °C for 5 minutes. For thorough mixing, pipette the entire reaction volume up and down 10 times or vortex sample for 30 seconds. These additional steps are most helpful for sample volumes larger than 50  $\mu$ l.
-

---

*Cutoff too close to target*

- **The cutoffs are not distinct.** For most efficient recovery, choose a cutoff as far removed from the desired fragments as possible.  
*E.g.*, If the desired fragments are around 500 bp and the undesired fragments are at 50 bp, choose the 100 bp cutoff for maximum retention of the desired fragment while completely depleting the undesired fragment. Choosing a higher cutoff results in diminished recovery of the desired fragments.

---

*Range of selection too small for double sided size selection*

- **Target region too small.** For a double-sided size selection, the recovery of a target region decreases significantly as the target region decreases. To maximize recovery of the target range, the two cutoffs should be as far apart as possible in order to increase the recovery of the target range.

---

**Low DNA Quality**

*Low 260/230*

- **Salt Contamination.** Ensure that both wash steps are performed to thoroughly remove any residual salt contamination. Incomplete washing will result in low 260/230 ratios.
  - **Ethanol Contamination.** To prevent ethanol contamination, remove as much DNA Wash buffer as possible before drying beads. Samples can be given a quick spin to bring down remaining buffer before transferring to magnetic rack to aspirate any residual buffer. Alternatively, allow samples to air dry at room temperature for 3 minutes before resuspending with **DNA Elution Buffer**.
-

# Appendix

## Automation Scripts

The **Select-a-Size DNA Clean & Concentrator™ MagBead Kit** is compatible with automated platforms. For automation scripts and related technical support, email [automation@zymoresearch.com](mailto:automation@zymoresearch.com). In the subject line, please include “Automation Scripts” and include the instrument used and the product catalog number.

# Ordering Information

Product Description	Catalog No.	Size
Select-a-Size DNA Clean & Concentrator™ MagBead Kit	D4084	10 ml
Select-a-Size DNA Clean & Concentrator™ MagBead Kit	D4085	50 ml

Individual Kit Components	Catalog No.	Amount
Select-a-Size MagBead	D4084-4-10 D4084-4-50	10 ml 50 ml
DNA Wash Buffer (concentrate)	D4003-2-24 D4003-2-48	24 ml 48 ml
DNA Elution Buffer	D3004-4-10 D3004-4-16 D3004-4-50	10 ml 16 ml 50 ml
Collection Plate	C2002	2 Plates
Elution Plate	C2003	2 Plates
96-Well Plate Cover Foil	C2007-2 C2007-4 C2007-8	2 Foils 4 Foils 8 Foils
ZR-96 MagStand	P1005	1 Stand



**100% satisfaction guarantee on all Zymo Research products,  
or your money back.**

Zymo Research is committed to simplifying your research with quality products and services. If you are dissatisfied with this product for any reason, please call 1(888) 882-9682.

---

Integrity of kit components is guaranteed for up to one year from date of purchase. Reagents are routinely tested on a lot-to-lot basis to ensure they provide the highest performance and reliability.

This product is for research use only and should only be used by trained professionals. It is not for use in diagnostic procedures. Some reagents included with this kit are irritants. Wear protective gloves and eye protection. Follow the safety guidelines and rules enacted by your research institution or facility.

™ Trademarks of Zymo Research Corporation



ZYMO RESEARCH

The **BEAUTY** of **SCIENCE** is to Make Things **SIMPLE**®



[tech@zymoresearch.com](mailto:tech@zymoresearch.com)



[www.zymoresearch.com](http://www.zymoresearch.com)



Toll Free: (888) 882-9682